



LAWRENCE
LIVERMORE
NATIONAL
LABORATORY

On-Chip Dielectrophoretic Separation and Concentration of Viable, Non-Viable and Viable but Not Culturable (VBNC) *Escherichia coli*

M. M. Packard, M. Shusteff, E. C. Alocilja

April 13, 2012

TechConnect World 2012 - Nanotech, Microtech, Biotech,
Cleantech Joint 2012 Conferences
Santa Clara, CA, United States
June 18, 2012 through June 21, 2012

Disclaimer

This document was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor Lawrence Livermore National Security, LLC, nor any of their employees makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or Lawrence Livermore National Security, LLC. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or Lawrence Livermore National Security, LLC, and shall not be used for advertising or product endorsement purposes.

On-Chip Dielectrophoretic Separation and Concentration of Viable, Non-Viable and Viable but Not Culturable (VBNC) *Escherichia coli*

Michelle M. Packard^a, Maxim Shusteff^b,
Evangelyn C. Alocilja^{*a}

^aNanobiosensors Laboratory, Michigan State
University, East Lansing, MI 48824;

^bLawrence Livermore National Laboratory, 7000
East Avenue, Livermore CA 94550

*alocilja@msu.edu, phone: (517) 432-8672,
www.msu.edu/~alocilja

This work partially performed under the auspices of the U.S.
Department of Energy by Lawrence Livermore National
Laboratory under Contract DE-AC52-07NA27344.
Release Number LLNL-CONF-548191.

ABSTRACT

Although bacterial culture remains the gold standard for detection of viable bacteria in environmental specimens, the typical time requirement of twenty-four hours can delay and even jeopardize appropriate public health intervention. In addition, culture is incapable of detecting viable but not culturable (VBNC) species. Conversely, nucleic acid and antibody-based methods greatly decrease time to detection but rarely characterize viability of the bacteria detected. Through selection by membrane permeability, the method described in this work employs positive dielectrophoresis (pDEP) for separation and purification of viable and VBNC species from water and allows concentration of bacteria for downstream applications.

Keywords: viable but not culturable (VBNC), *Escherichia coli* C3000, bacterial viability, ATP production, membrane integrity, metabolic capacity

1 INTRODUCTION

During disinfection or in the presence of a stress environment, bacteria may enter a viable but non-culturable (VBNC) state in which growth and replication ceases but viability and pathogenicity are maintained [1-4]. This unique quality increases the need for an assay which can reliably and specifically detect viable organisms without cultivation. The VBNC state has been induced under a number of conditions including low temperatures, starvation, and in the presence of certain chemicals. Bacteria in this state are characterized by an inability to form colonies under standard plating procedures while maintaining an intact membrane capable of preventing the uptake of certain dyes such as propidium

iodide. Confirmation of viability can be achieved through resuscitation in specialized broth media [5-8]. Separation and concentration of viable bacteria by dielectrophoresis (DEP) has previously been demonstrated [9-13], however, to date, no research has been done to characterize the behavior of viable but not culturable (VBNC) *Escherichia coli* species in the presence of high frequency electric fields. A key parameter governing the effect of such fields is the Clausius-Mossotti factor (F_{CM}). In positive dielectrophoresis, $\text{Re}[F_{CM}]$ is greater than 0 and the dielectrophoretic constant of the particle is greater than that of the medium; here, the particle moves “up the field gradient” toward regions of greatest electric field. In negative dielectrophoresis, $\text{Re}[F_{CM}]$ is less than 0 and the dielectrophoretic constant of the particle is less than that of the medium so the particle moves toward regions of lowest field. Upon cell death and subsequent membrane permeability, cell conductivity increases by $\sim 10^4$ as inner cell composition more closely resembles that of the surrounding medium, resulting in a greater $\text{Re}[F_{CM}]$.

The dielectrophoretic force (F) experienced by a given colloidal particle can be approximated by equation (1) for spherical particles, where ϵ_0 =vacuum dielectrophoretic constant, r =particle radius, E_{rms} =root mean square value of electric field, $\text{Re}[F_{CM}]$ is the real part of the Clausius-Mossotti factor (equation 2), ϵ_p^* =relative permittivity of particle, and ϵ_m^* =relative permittivity of medium.

$$F = 2\pi\epsilon_0\epsilon_m r^3 \text{Re}[F_{CM}] \nabla |E_{rms}|^2 \quad (1)$$

$$\text{Re}[F_{CM}] = (\epsilon_p^* - \epsilon_m^*) / (\epsilon_p^* + 2\epsilon_m^*) \quad (2)$$

Because dielectrophoretic separation of live and dead *Escherichia coli* is dependent on various cell morphologies and components including its non-spherical shape, a model was experimentally generated to predict the behavior of bacteria when subjected to various media and frequencies. These factors were then tested to compare the behavior of VBNC species to that of live and dead cells.

2 MATERIALS AND METHODS

2.1 Bacterial Preparation

Escherichia coli C3000 (ATCC# 15597) was grown overnight at 37°C in nutrient broth then centrifuged at 3000 rpm for five minutes and rinsed three times in distilled water (dH₂O). The resulting pellet was then resuspended and incubated for six days in one of the following:

- Nutrient broth at 37°C
- 70% Isopropanol (IPA)
- 0.5, 5, 50 or 500 μM copper sulfate (CuSO_4) in 0.9% NaCl at 25°C (to induce VBNC)

After incubation, samples were centrifuged at 3000 rpm for five minutes, then rinsed three times in dH₂O for culture and membrane integrity testing in Brain Heart Infusion (BHI) broth, and finally incubated at 37°C for 24 hours to

resuscitate. Samples were assayed for culturability, cell membrane integrity, and ability to resuscitate prior to initial resuspension and after six days incubation in nutrient broth, IPA, or CuSO₄. To determine limits of detection, samples were then serially diluted from 10⁻¹ to 10⁻⁸ in either dH₂O or BHI broth. All testing was completed in triplicate.

2.2 Induction and confirmation of VBNC

To quantify levels of untreated bacteria, 100 μ L of bacteria diluted to 10⁻⁴ in dH₂O was plated on MacConkey agar with sorbitol (SMAC). At days 2 and 6, 100 μ L of each sample was also plated undiluted to assess loss of culturability. Serial dilutions of resuscitated bacteria were also plated to verify expected concentrations and derive calibration curves for viability assay.

Membrane integrity was observed with the LIVE/DEAD BacLight bacterial viability assay (Promega Cat No. L7012). A 2X solution consisting of 1 μ L 3.34 mM Syto 9 and 1 μ L 20 mM propidium iodide in 1 mL dH₂O was mixed with equal parts of each sample. Viable cells were then excited using a QBC ParaLens Advance LED objective consisting of a blue LED (385-480 nm) for excitation and a longpass filter (>510 nm) to view both viable (green) and nonviable (red) cells. Ten images were captured for each sample and cells were counted manually.

2.3 Dielectrophoretic Separation and Detection

Dielectrophoresis was performed on a modified flow array (Fig. 1) customized by Applied Biophysics (Part No 8F10E, Troy, NY). Normally configured with 10 active 250 μ m diameter electrodes per region (Fig. 2), photoresist was omitted during fabrication to produce eight individually addressable electrodes per array at the base of the 100 μ L flow channel (50 mm x 5 mm x 0.4 mm). Alternating current (10 V_{p-p}) was applied to the electrode via a laptop-controlled frequency generator (Velleman, Inc PCGU1000). Flows from 3 mL luer-lock syringe were controlled using a syringe pump (New Era NE1000). For the purposes of this work, a small region centered on the electrode edge was visualized by LED microscopy with a 20X objective. Images were captured by a ScopeTek 2.0M pixel CCD camera and MiniSee software and analyzed with ImageJ software for background subtraction[14].

To determine the parameters for optimal separation of live and dead *Escherichia coli*, dielectrophoresis was initially performed at a range of frequencies in 10⁻⁵ to 10⁻² concentrations of PBS diluted in deionized water (conductivities = 2.7, 3.2, 15.46, and 154.0, μ S/cm, respectively) and flowed for 50 μ L/min for two minutes for each frequency tested. An image was then captured at the conclusion of the flow period and manually counted in two regions, at the electrode edge and nearing the electrode center. Counts at the former (pDEP) and latter (nDEP) were represented as a percentage of all cells collected for both live and dead populations (pDEP % and nDEP%). An estimate of

the dominating DEP force was then derived by equation (3) for live and dead populations at each tested frequency. Bacteria treated with 500 μ M CuSO₄ in 0.9% NaCl were then separately but identically subjected to dielectrophoretic conditions to assess their behavior as compared to live and dead bacteria.

$$\text{DEP\%} = \text{pDEP\%} - \text{nDEP\%} \quad (3)$$

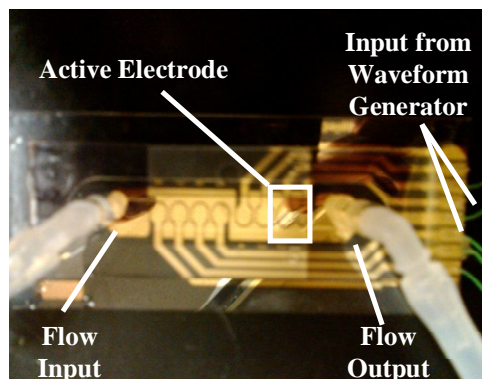


Figure 1. Modified Applied Biophysics flow array employed for bacterial dielectrophoresis.

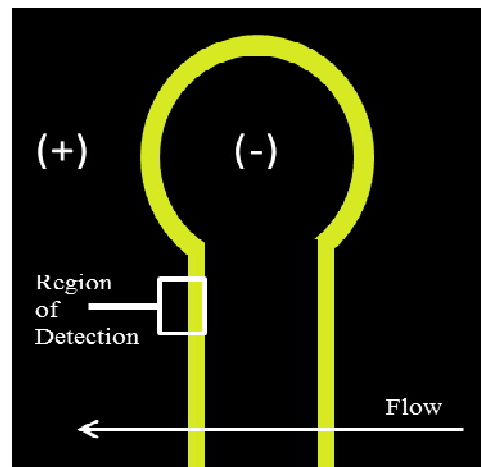


Figure 2. Illustration of single electrode within the flow array.

3 RESULTS AND DISCUSSION

3.1 Viability Testing

Plating results revealed initial bacterial concentration equal to 5 x 10⁷ cfu/mL. Limit of detection as determined by lowest dilution producing colonies was 10⁻⁶, equivalent to 50 cfu/mL. Limit of detection for the LIVE/DEAD assay was 10⁵ cfu/mL. A linear relationship comparing viable cell counts and culture results was statistically significant (R²=0.9943) for concentrations ranging from 10⁵-10⁷. At concentrations greater than 10⁷, cells were too numerous to accurately count. At concentrations below 10⁵, no cells were detectable. Within the linear range, each cell in the observation region

could be extrapolated to represent 2.1×10^6 cells/mL ($R^2=0.9805$). This relationship was used to estimate concentrations of viable cells for CuSO_4 treated samples.

3.2 Induction and detection of VBNC

For CuSO_4 treated samples, 0.5 and 5 μM CuSO_4 were found to have no significant effect on culturability or viability as compared to normal growth. At 50 μM CuSO_4 , the number of culturable cells decreased by a factor of approximately 10^3 , however no significant decrease in viable cells was noted. At 500 μM CuSO_4 , culture resulted in no colonies, however, the presence of cells with compromised membranes was scarce (Figures 3a and b).

Comparatively, the membranes of cells incubated in IPA were compromised throughout the population. Treatment with IPA resulted in full removal of both culturable and viable cells within two days incubation (Figure 3c), and this loss remained following the resuscitation procedure. The sample incubated in BHI at 37°C showed minimal variation in viability and culturable (10^8 - 10^9 cfu/mL) over six days or after the resuscitation procedure. However, 500 μM CuSO_4 reduced culturability by approximately 10^3 cfu/mL after two days incubation and completely after six days. Despite this, the number of viable cells in 500 μM CuSO_4 decreased but only to about 10^6 cfu/mL after six days. The resuscitation procedure was successful, with both culturable and viable cell counts resuming to $>10^8$, in good agreement with the positive control. Despite lacking in culturability, viable cell counts for these treated samples stained with LIVE/DEAD assay were equivalent to 10^6 cells/mL. After resuscitation, cell levels as determined by culture and membrane integrity were all approximately 10^8 cells/mL.

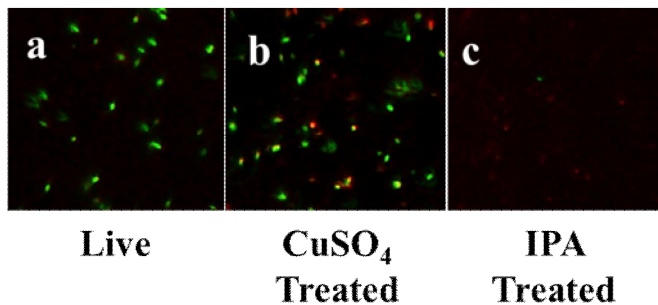


Figure 3. Visualization of intact membranes as indicated by LIVE/DEAD viability assay. A) Live, untreated cells showed were fully viable with maintained membranes (green). B) After treatment with CuSO_4 , a scarce number of cells demonstrated compromised membranes (red) however the majority are intact. C) Treatment with IPA resulted in compromised membranes for all but one cell.

3.3 Dielectrophoretic Separation and Detection

When resuspended in 10^{-5} PBS (3.2 $\mu\text{S}/\text{cm}$), both live and dead cells behaved similarly, demonstrating pDEP at

frequencies greater than 1 kHz. Cell separation was achieved in both 10^{-3} and 10^{-4} PBS (Figure 4). Here, pDEP was noted for live cells at frequencies above 23 and 4 kHz, respectively, while nDEP remained dominant for dead cells up to 41 and 6 kHz, respectively. No dielectrophoresis was observed in 10^{-2} PBS (Figure 4). Because the largest range of frequencies under which separation could be observed was detected with 10^{-3} PBS, this media was used exclusively for subsequent VBNC studies.

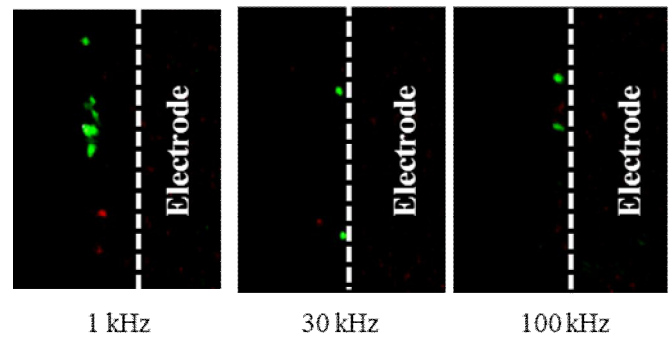


Figure 4. Dielectrophoresis of live and dead bacteria in 10^{-3} PBS. At 1 kHz, both live and dead bacteria were repelled away from the electrode edge (white dotted line), indicative of dominating nDEP forces. At 30 kHz, dead bacteria remained under nDEP forces while live bacteria were attracted to the electrode edge (pDEP). At 100 kHz, both live and dead bacteria were subjected to pDEP forces.

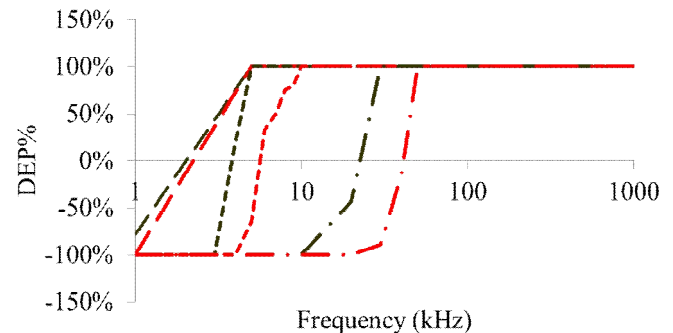


Figure 5. Dielectrophoretic behavior of live (green) and dead (red) cells for 10^{-5} (—), 10^{-4} (---), and 10^{-3} (— · —) PBS. DEP% less than zero is indicative of nDEP whereas DEP% greater than zero suggests pDEP.

CuSO_4 -induced VBNC suspended in 10^{-3} PBS behaved almost identically to live cells, with nDEP observed for lower frequencies and pDEP occurring at frequencies above 20 kHz (Figures 6 and 7). This initial data suggests that dielectrophoresis may offer a simple and predictive mechanism for isolation of viable cells regardless of culturability.

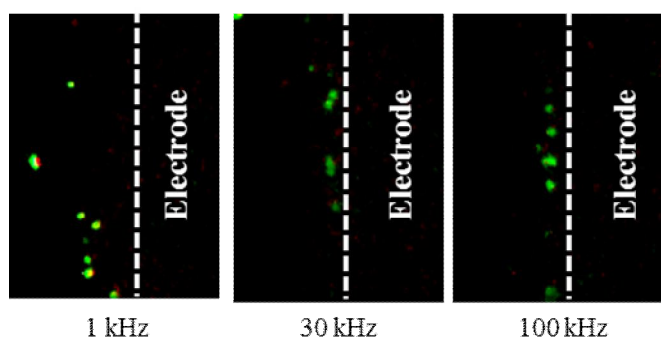


Figure 6. Dielectrophoresis of VBNC. Similar to live bacteria, VBNC bacteria displayed nDEP at 1 kHz and pDEP for frequencies greater than 20 kHz.

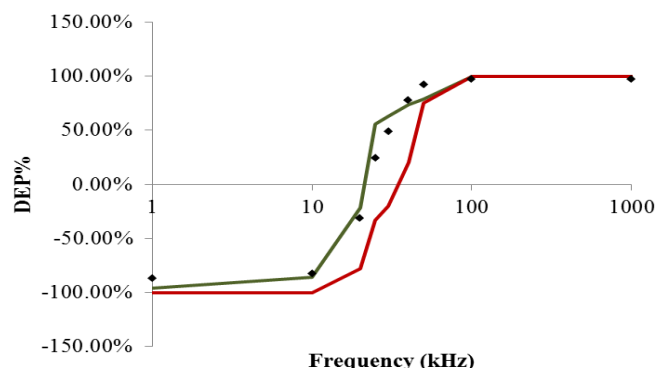


Figure 7. DEP% for both live (green) and dead (red) bacteria was negative in the range of 1-10 kHz. The crossover frequencies for live and dead bacteria were 23 kHz and 41 kHz, respectively. Above the crossover, all bacteria were positively attracted to the electrode edge. Dynamics and crossover frequencies of VBNC species (•) were consistent with those of live bacteria.

4 CONCLUSIONS

The VBNC state, determined by comparison of culture and membrane integrity, was successfully induced by incubation in 500 μM CuSO_4 . Bacteria in this state were determined undetectable by culture but were successfully resuscitated to initial concentration. Upon determining the optimal conditions for cell separation, an assessment of the dielectrophoretic behavior of VBNC cells revealed behavior most similar to that of live cells. Based on this data, we suggest that dielectrophoresis may be a reliable and more suitable mechanism for viable cell isolation, especially where concerns of VBNC presence are of issue. Although further trials will be necessary to explore the breadth to which these results are applicable, this initial report shows promise for this technological application.

REFERENCES

- [1] N. H. Keep, J. M. Ward, G. Robertson, M. Cohen-Gonsaud, and B. Henderson, "Bacterial resuscitation factors: revival of viable but non-culturable bacteria," *Cell Mol Life Sci*, vol. 63, pp. 2555-9, 2006.
- [2] T. Nystrom, "Not quite dead enough: on bacterial life, culturability, senescence, and death," *Arch Microbiol*, vol. 176, pp. 159-64, 2001.
- [3] T. Nystrom, "Conditional senescence in bacteria: death of the immortals," *Mol Microbiol*, vol. 48, pp. 17-23, 2003.
- [4] T. Nystrom, "Nonculturable bacteria: programmed survival forms or cells at death's door?," *Bioessays*, vol. 25, pp. 204-11, 2003.
- [5] V. Besnard, M. Federighi, and J. M. Cappelletti, "Development of a direct viable count procedure for the investigation of VBNC state in *Listeria monocytogenes*," *Lett Appl Microbiol*, vol. 31, pp. 77-81, 2000.
- [6] Y. Wang, L. Claeys, D. van der Ha, W. Verstraete, and N. Boon, "Effects of chemically and electrochemically dosed chlorine on *Escherichia coli* and *Legionella beliardensis* assessed by flow cytometry," *Appl Microbiol Biotechnol*, vol. 87, pp. 331-41, 2010.
- [7] A. Rompre, P. Servais, J. Baudart, M. R. de-Roubin, and P. Laurent, "Detection and enumeration of coliforms in drinking water: current methods and emerging approaches," *J Microbiol Methods*, vol. 49, pp. 31-54, 2002.
- [8] G. Gregori, S. Citterio, A. Ghiani, M. Labra, S. Sgorbati, S. Brown, and M. Denis, "Resolution of viable and membrane-compromised bacteria in freshwater and marine waters based on analytical flow cytometry and nucleic acid double staining," *Appl Environ Microbiol*, vol. 67, pp. 4662-70, 2001.
- [9] R. Pethig and G. H. Markx, "Applications of dielectrophoresis in biotechnology," *Trends Biotechnol*, vol. 15, pp. 426-32, 1997.
- [10] L. Yang, P. P. Banada, A. K. Bhunia, and R. Bashir, "Effects of Dielectrophoresis on Growth, Viability and Immuno-reactivity of *Listeria monocytogenes*," *J Biol Eng*, vol. 2, pp. 6, 2008.
- [11] B. Lapizco-Encinas, Simmons, BA, Cummings, EB, Fintschenko, Y, "Dielectrophoretic Concentration and Separation of Live and Dead Bacteria in an Array of Insulators," *Anal Chem*, vol. 76, pp. 1571-1579, 2004.
- [12] M. D. Pysher and M. A. Hayes, "Electrophoretic and dielectrophoretic field gradient technique for separating bioparticles," *Anal Chem*, vol. 79, pp. 4552-7, 2007.
- [13] J. Voldman, "Electrical forces for microscale cell manipulation," *Annu Rev Biomed Eng*, vol. 8, pp. 425-54, 2006.
- [14] M. D. Abramoff, Magalhaes, P.J., Ram, S.J., "Image Processing with ImageJ," *Biophotonics International*, vol. 11, pp. 36-42, 2004.